VitaGuard® VG 310 – short instructions

This instruction leaflet does not replace the manual. If you are not familiar with the manual, the patient's health may be at risk. Please take sufficient time to read the manual.

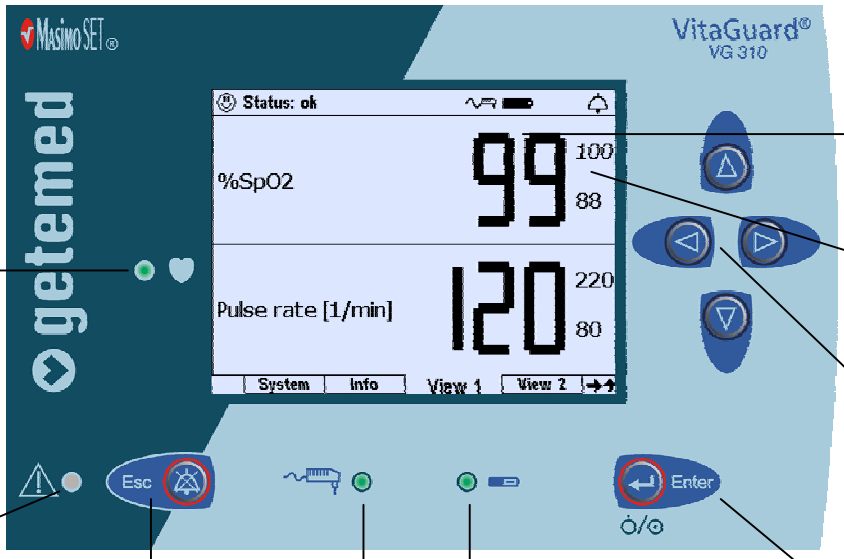

LED flashes synchronously with pulse

Current value of the respective vital function

Currently set alarm limits

Navigation keys

LED „Alarm" flashes red for physiological and yellow for technical alarm.

LED "External power adapter"

LED "Rechargeable battery is loading"

<Enter> key for switching on and confirming settings

<Esc> key for pausing the acoustic alarm and to exit menus

Summary of steps before monitoring

- Insert the battery or batteries (do not switch on yet!).
- Use the external power adapter to connect VitaGuard® to the supply network (do not switch on yet!).
- Attach the SpO_2 sensor to the patient.
- Connect the SpO_2 patient cable to VitaGuard®.
- Connect the SpO_2 sensor to the patient cable.
- Switch on VitaGuard®.

Make sure that after the monitor is switched on the indicator lamps light up briefly and a short sound is emitted by the alarm buzzers.

Check that the alarm limits displayed are the same as those recommended by the doctor.

Switching off VitaGuard®

Always switch off VitaGuard® in the manner described here.

1 Press the <Enter> key and keep this pressed: the message PRESS ESC KEY appears.

2 Briefly press the <Esc> key, still keeping the <Enter> key pressed, and then release both keys.

The switch off command is acknowledged by two short beeps.

Data must be stored before the device finally switches off. For this reason, VitaGuard® needs about another two seconds after the keys are released until it switches off completely.

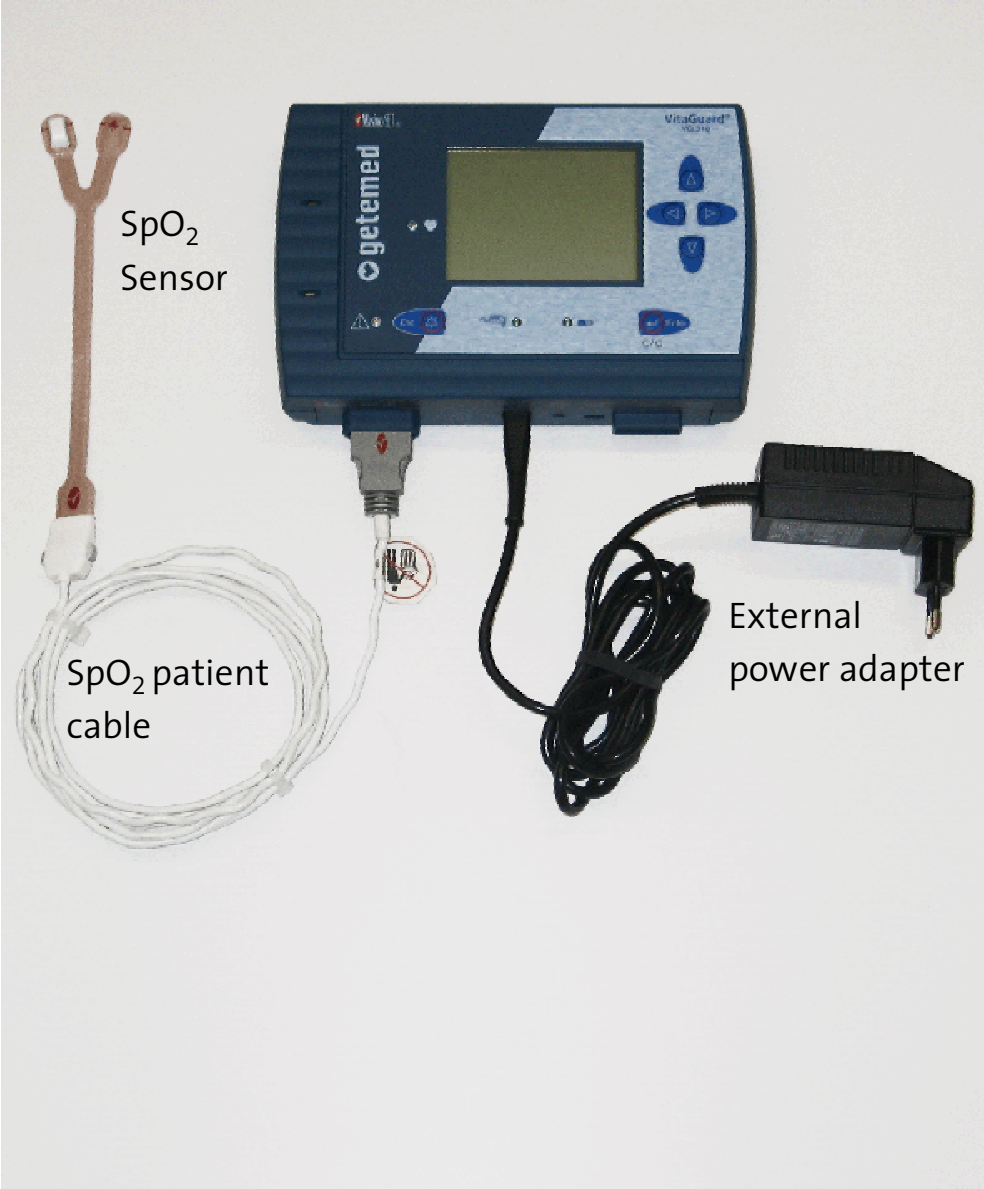
SpO_2
Sensor
SpO_2 patient
cable
External
power adapter

Distributor:

Manufacturer:

getemed
Medizin- und Informationstechnik AG
Oderstraße 77
D-14513 Teltow

Tel.	+49 (0) 33 28 39 42- 0
Fax	+49 (0) 33 28 39 42-99
E-Mail	info@getemed.de
Internet	www.getemed.de

REF-Nr.:.7382 3021 0027H1-LAB-Rev-A-VitaGuard-VG310-Kurz-GA-ENG.doc 8/24/2005 2:21

getemed